


# Minimum / maximum temperature chart

VSP Number \_\_\_\_\_

Location of Refrigerator \_\_\_\_\_

Month and Year \_\_\_\_\_ / \_\_\_\_\_

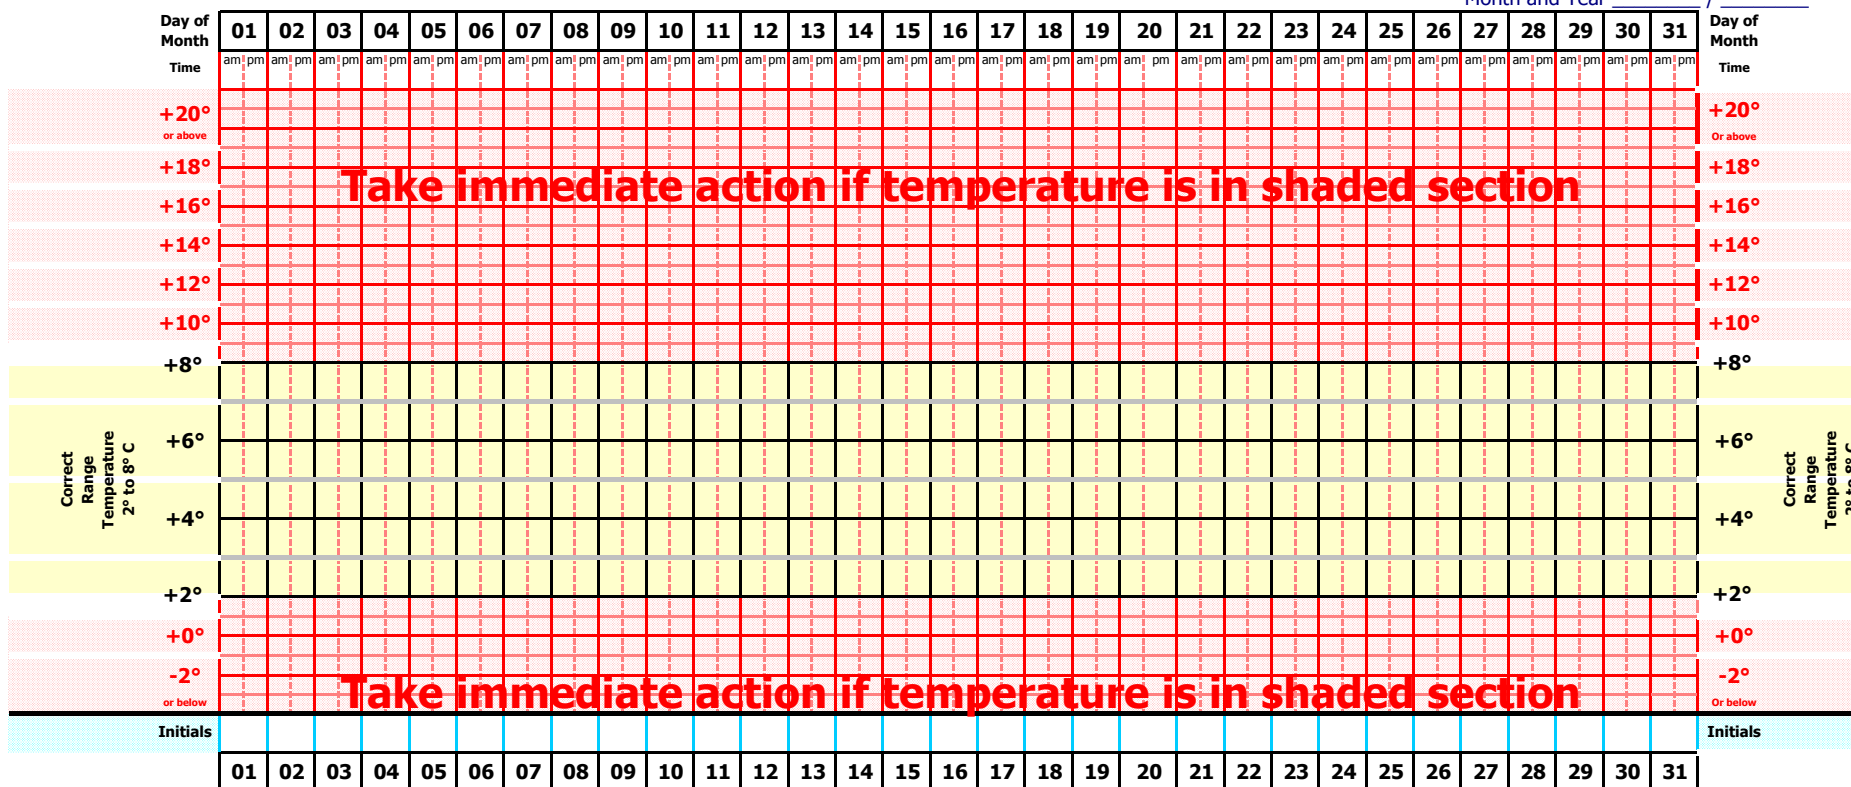

Mark minimum and maximum temperatures on the graph with a black pen twice daily

Date \_\_\_/\_\_\_/\_\_\_ Audited by: \_\_\_\_\_ Cleaning Date \_\_\_/\_\_\_/\_\_\_

## Maintaining and monitoring refrigerator temperatures

- 🔧 Check and record the minimum and maximum temperature on the graph twice daily before vaccination and at clinic/practice closure. RESET THE THERMOMETER IF DOMESTIC REFRIGERATOR after recording.
- 🔧 Store vaccines between +2° to +8°C (strive for 5). The red shaded zones represent immediate action.
- 🔧 Check temperature every time you open your refrigerator.
- 🔧 Retain a copy of your minimum/maximum recordings according to organisation policy or advice from the principal doctor's medical defence organisation.

- If the temperature recorded is in the red shaded zone.**
1. Isolate vaccines - store vaccine between +2° to +8°C as quickly as possible.
  2. Do not discard vaccines.
  3. Call QHIP on **3234 1500** as soon as possible in business hours.
  4. Document action taken on the Vaccine Storage Troublesheet.

